
Display Report

Analysis Info

Analysis Name	D:\Data\AC\AHP\Conrads\CC-408-SN-APCI-pos-3.d	Acquisition Date	6/12/2023 10:01:47 AM
Method	APCI-kleine Massen-2-06.06.2023.m	Operator	Demo User
Sample Name	CC-408-SN	Instrument	maXis II 1828979.22385
Comment	MeOH		

Acquisition Parameter

Source Type	APCI	Ion Polarity	Positive	Set Nebulizer	3.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	220 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	3000 m/z	Set Charging Voltage	0 V	Set Divert Valve	Source
		Set Corona	4000 nA	Set APCI Heater	250 °C

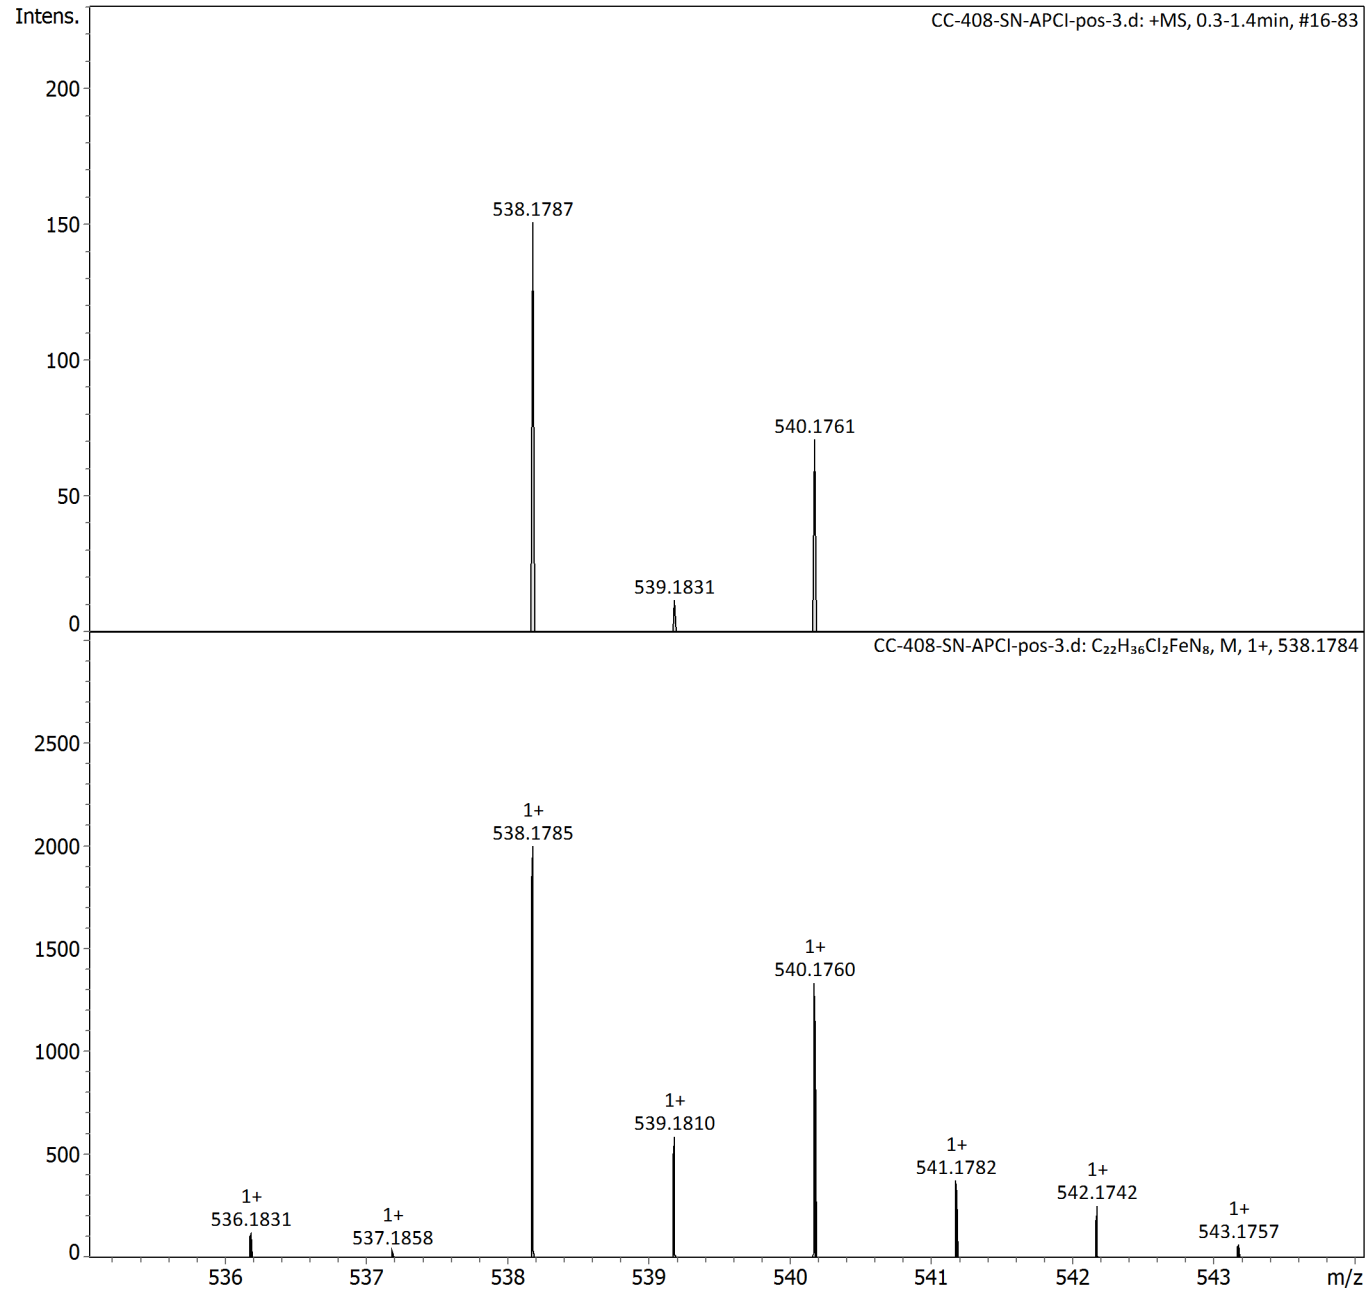

CC-408-SN-APCI-pos-3.d