Agilent Technologies

Sample ID:JAU-R5

Method Name:C:\Users\Public\Documents\Agilent\MicroLab\Methods\Default.a2m

Sample Scans:32

User:Student

Background Scans:32

Date/Time:09.29.2025 10:20:21


Resolution:4

Range:4000 - 650

System Status:Good

Apodization:Happ-Genzel

File Location:C:\Users\Public\Documents\Agilent\MicroLab\Results\\JAU-R5_2025-09-29T10-20-21.a2r

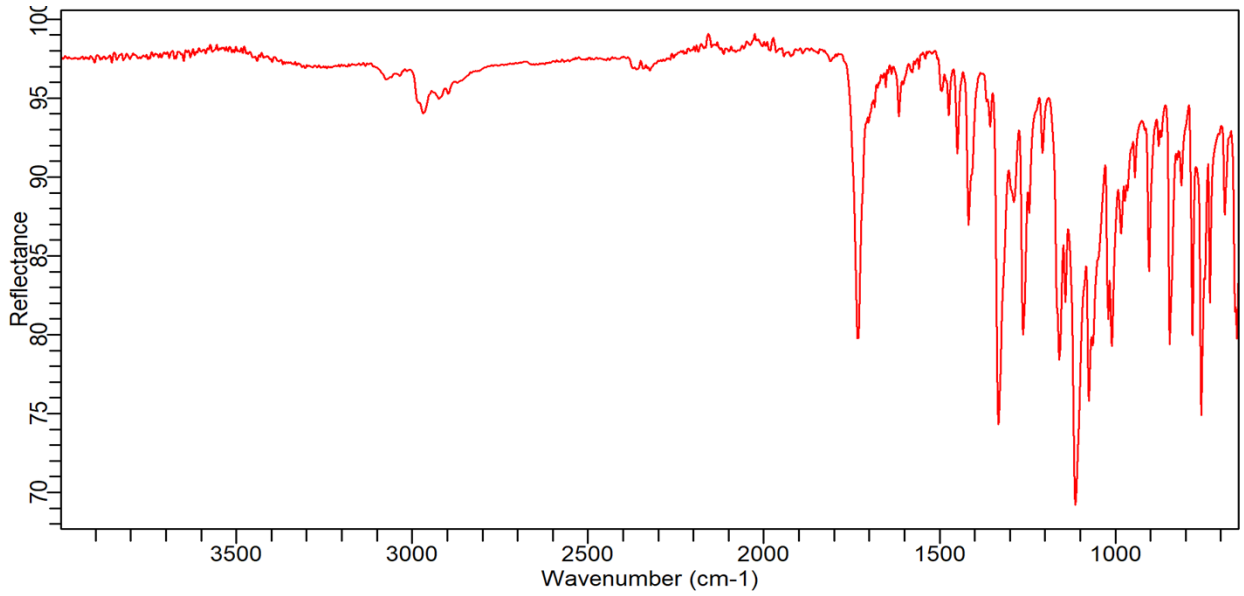

Peak Number	Wavenumber (cm^{-1})	Intensity